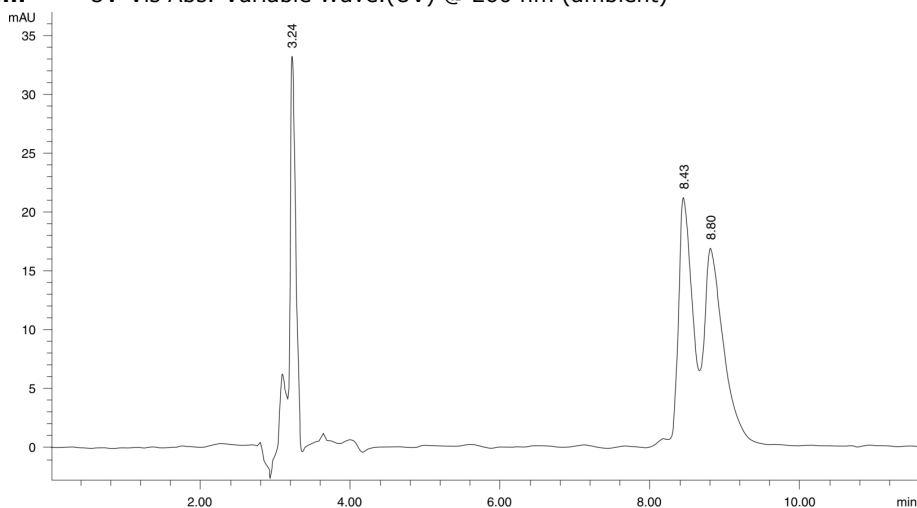


Cyclopentolate

Column: N/A**Dimensions:** N/A**Order No:** N/A**Elution Type:** N/A**Eluent A:** Hexane/Dichloroethane/Ethanol-TFA (55:35:10) ethanol-TFA 20:1**Gradient**

Profile:	Step No.	Time (min)	Pct A
1	1	0	100

Flow Rate: 1 mL/min**Col. Temp.:** ambient**Detection:** UV-Vis Abs.-Variable Wave.(UV) @ 260 nm (ambient) $\alpha = 1.07$

ANALYTES:

- 1** Cyclopentolate
Retention Time: 3.24 min
- 2** Cyclopentolate
Retention Time: 8.43 min
- 3** Cyclopentolate
Retention Time: 8.8 min

