

HPLC Application


ID No.: 13675

Nicotine

Column: N/A
Dimensions: N/A
Order No: N/A
Elution Type: N/A
Eluent A: Hexane/Dichloroethane/Ethanol-TFA (55:35:10) ethanol-TFA 20:1
Gradient

Step No.	Time (min)	Pct A
1	0	100

Flow Rate: 1 mL/min
Col. Temp.: ambient
Detection: UV-Vis Abs.-Variable Wave.(UV) @ 260 nm (ambient)

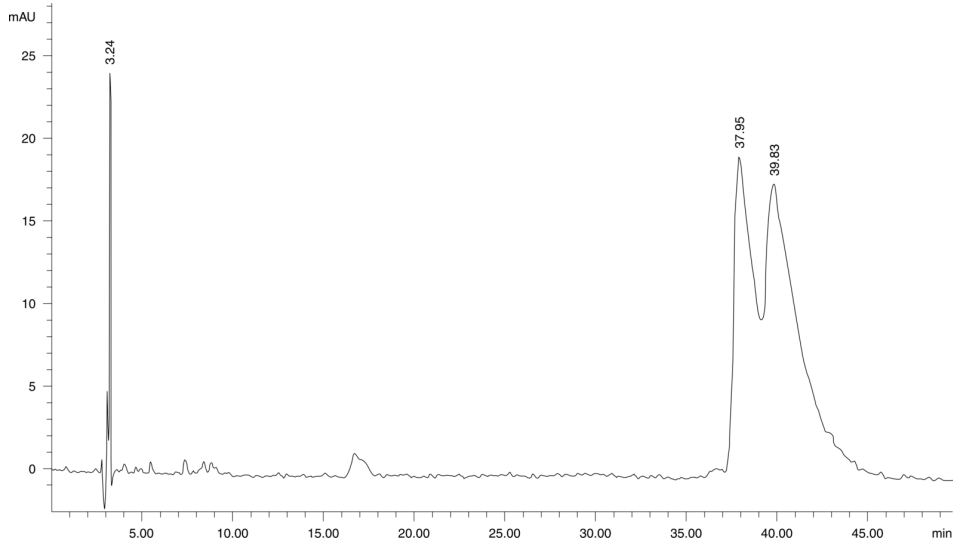

ANALYTES:

- 1 Nicotine
Retention Time: 37.95 min
- 2 Nicotine
Retention Time: 39.83 min

