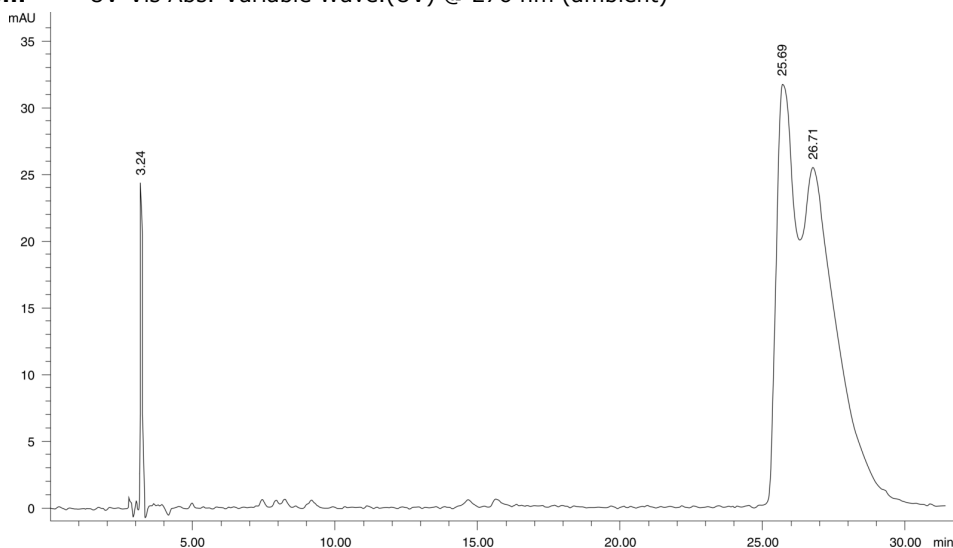


Octopamine

Column: N/A**Dimensions:** N/A**Order No:** N/A**Elution Type:** N/A**Eluent A:** Hexane/Dichloroethane/Ethanol-TFA (55:35:10) ethanol-TFA 20:1**Gradient**

Profile:	Step No.	Time (min)	Pct A
	1	0	100

Flow Rate: 1 mL/min**Col. Temp.:** ambient**Detection:** UV-Vis Abs.-Variable Wave.(UV) @ 276 nm (ambient)

ANALYTES:

1 Octopamine

Retention Time: 3.24 min

2 Octopamine

Retention Time: 25.69 min

3 Octopamine

Retention Time: 26.71 min

