

# HPLC Application

ID No.: 14748

## Oligosaccharide Std. (AL0-3038)

**Column:** Rezex<sup>™</sup> RSO-Oligosaccharide Ag+ 4%, LC Column 200 x 10 mm, Ea

**Dimensions:** 200 x 10 mm ID

**Order No:** 00P-0133-N0

**Elution Type:** Isocratic

**Eluent A:** Water

| Gradient | Step No. | Time (min) | Pct A |
|----------|----------|------------|-------|
| Profile: | 1        | 0          | 100   |

**Flow Rate:** 0.3 mL/min

**Col. Temp.:** 85 °C


**Detection:** Refractive Index (RI) @ nm (85 °C)

**Analyst Note:** This standard is used to test the following HPLC columns: REZEX RSO (Ag Oligosaccharide) and RNO (Na Oligosaccharide)

NOTE: Separation conditions and results may vary for your column. Contact your Technical Representative.



Products used in this application:

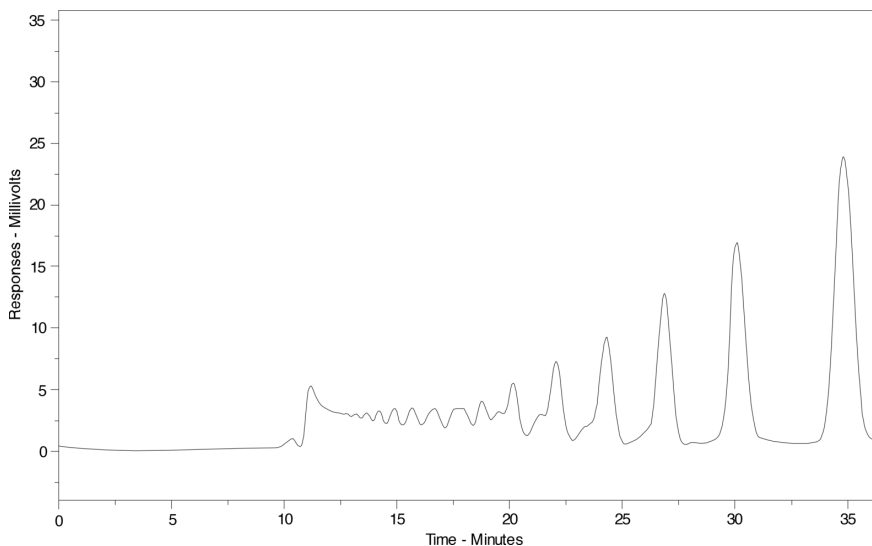

### ANALYTES:

- 1 Light corn syrup

