

## Anion-Exchange Std. (AL0-3041)

**Column:** PhenoSphere™ 5 µm SAX 80 Å, LC Column 250 x 4.6 mm, Ea

**Dimensions:** 250 x 4.6 mm ID

**Order No:** 00G-3151-E0

**Elution Type:** Isocratic

**Eluent A:** 0.15M (NH<sub>4</sub>)<sub>2</sub> HPO<sub>4</sub>, pH 6.0

Gradient	Step No.	Time (min)	Pct A
Profile:	1	0	100

**Flow Rate:** 0.6 mL/min

**Col. Temp.:** ambient

**Detection:** UV-Vis Abs.-Variable Wave.(UV) @ 254 nm (ambient)


**Analyst Note:** This standard is used to test the following Phenomenex silica-based ion-exchange columns:  
SAX, SB, DEAE, PEI.

NOTE: Separation conditions and results may vary for your column. Contact your Technical Representative.



Products used in this application:

**PhenoSphere™**

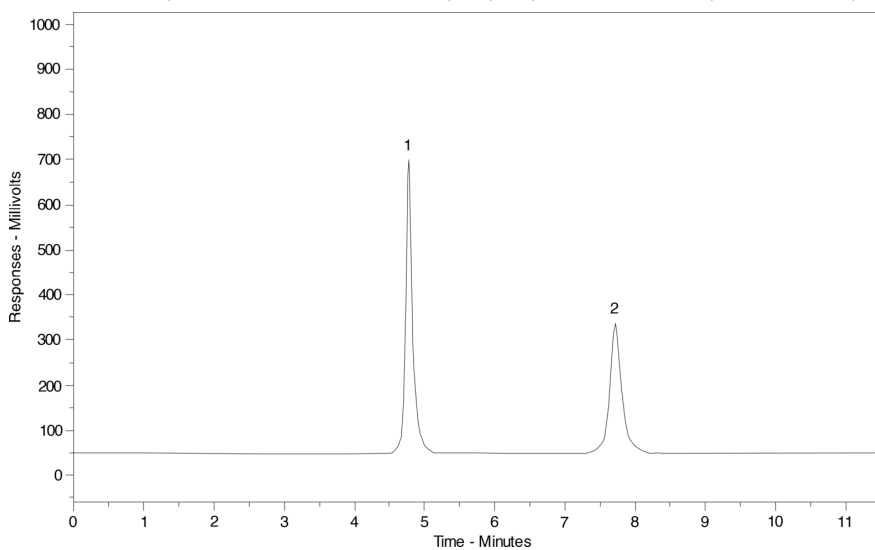

### ANALYTES:

**1** Uridine

Retention Time: 4.8 min

**2** UMP

Retention Time: 7.73 min

