

# HPLC Application

ID No.: 18467

## Calibration Curve for Melamine Extraction (20-2000ng/mL range) from Strata Melamine on Luna HILIC

**Column:** Luna® 3 µm HILIC 200 Å, LC Column 100 x 2 mm, Ea

**Dimensions:** 100 x 2 mm ID

**Order No:** 00D-4449-B0

**Elution Type:** Isocratic

**Eluent A:** 90/10 ACN/100 mM Ammonium Formate, pH 3.2

Gradient	Step No.	Time (min)	Pct A
<b>Profile:</b>	<b>1</b>	3.5	100

**Flow Rate:** 0.4 mL/min

**Col. Temp.:** ambient

**Detection:** Mass Spectrometer (MS) @ (ambient)

**Detector Info:** \* MS in -ve ionization till 1.7 mins then to +ve till 3.5 mins

**Analyst Note:** LC/MS/MS Condition:

Column: Luna 3µm HILIC, 100x2.0mm; Flow rate: 0.4ml/min

Mobile Phase: Isocratic; 90/10 ACN/100mM NH<sub>4</sub> Formate pH 3.2; MS Detector: API 3000 LC/MS/MS with ESI (TurboIonSpray®) (www.Appliedbiosystems.com), Switch from -ve Ion Mode (for cyanuric) to Positive Ion (for Melamine); MRM; heater gas flow 7000 cc/min; heater temperature 450 °C

Melamine QC - 200 ng

% Accuracy 99.45%

% CV 6%

Calibration Curve of Extracted Samples


conc. (ng)	% Accuracy
20	102%
40	96%
200	104%
400	98%
2000	100.03%



Products used in this application:



## Calibration Curve for Melamine Extraction (20-2000ng/mL range) from Strata Melamine on Luna HILIC

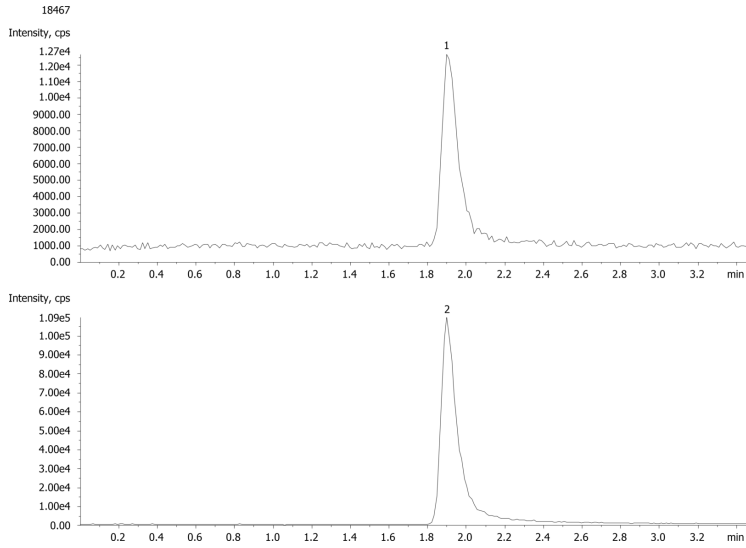

### ANALYTES:

- 1** Melamine  
Retention Time: 1.9 min
- 2** Melamine 13C3-Amino 15N3  
Retention Time: 1.9 min

