

HPLC Application

ID No.: 18566

QC Test Chromatogram (Agilent 1200SL) - Kinetex 2.6µm C18 50 x 2.1mm ID


Column: Kinetex® 2.6 µm C18 100 Å, LC Column 50 x 2.1 mm, Ea
Dimensions: 50 x 2.1 mm ID
Order No: 00B-4462-AN
Elution Type: Isocratic
Eluent A: Acetonitrile
Eluent B: Water
Gradient

Step No.	Time (min)	Pct A	Pct B
1	0	50	50

Profile:
Flow Rate: 0.49 mL/min
Col. Temp.: ambient
Detection: UV-Vis Abs.-Variable Wave.(UV) @ 254 nm (ambient)



Products used in this application:

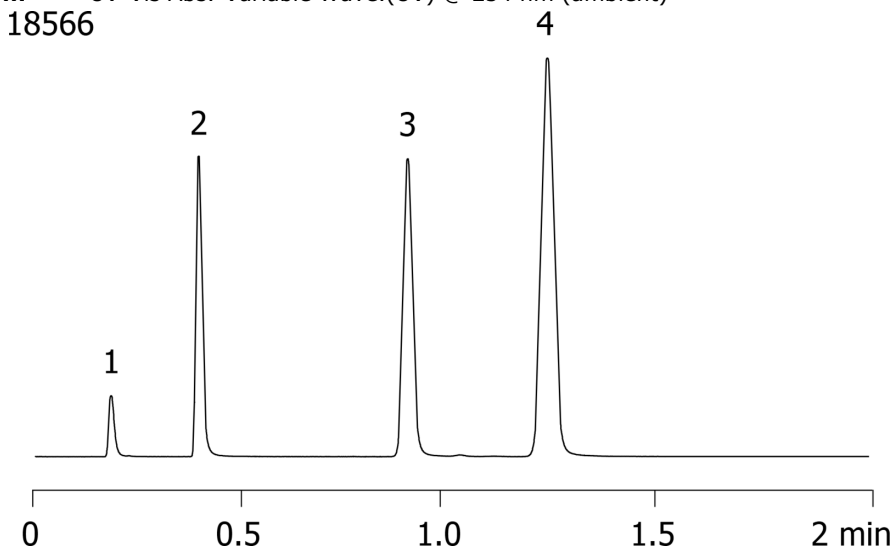

ANALYTES:

- 1** Uracil
Retention Time: 0.19 min
- 2** Acetophenone
Retention Time: 0.4 min
- 3** Toluene
Retention Time: 0.89 min
- 4** Naphthalene
Retention Time: 1.23 min

