

GFC Standard on BioSep-SEC-s2000 (AL0-3042)

Column: BioSep™ 5 µm SEC-s2000 145 Å, LC Column 300 x 7.8 mm, Ea

Dimensions: 300 x 7.8 mm ID

Order No: 00H-2145-K0

Elution Type: Isocratic

Eluent A: 100 mM PO4 Buffer pH 6.8/ 0.025% Na N3

| Gradient | Step No. | Time (min) | Pct A |
|-----------------|----------|------------|-------|
| Profile: | 1 | 0 | 100 |

Flow Rate: 1 mL/min

Col. Temp.: ambient


Detection: UV-Vis Abs.-Variable Wave.(UV) @ 280 nm (ambient)

Analyst Note: SecurityGuard™ Guard Cartridge System extends column lifetime.


- SecurityGuard Cartridges, GFC-2000 4 x 3.0mm ID, 10/Pk Part No.: AJ0-4487

- Holder Part No.: KJ0-4282

19806



Products used in this application:

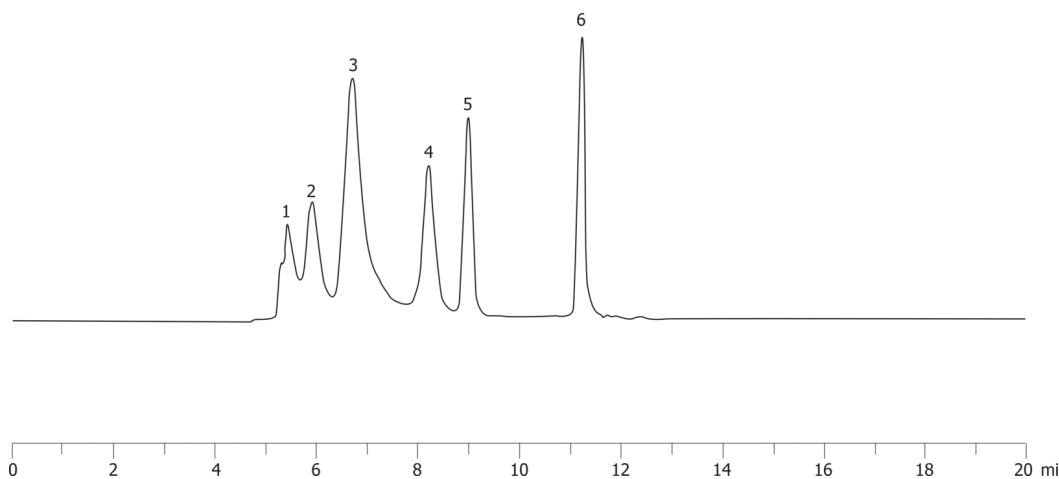

ANALYTES:

1 Bovine Thyroglobulin

Retention Time: 5.3 min

2 IgA

Retention Time: 5.93 min

3 IgG

Retention Time: 6.7 min

4 Ovalbumin

Retention Time: 8.21 min

5 Myoglobin

Retention Time: 9 min

6 Uridine

Retention Time: 11.23 min

