

GFC Standard on BioSep-SEC-s2000 (AL0-3042)

Column: BioSep[™] 5 μ m SEC-s2000 145 Å, LC Column 300 x 7.8 mm, Ea

Dimensions: 300 x 7.8 mm ID

Order No: 00H-2145-K0

Elution Type: Isocratic

Eluent A: 100 mM PO4 Buffer pH 6.8/ 0.025% Na N3

Gradient	Step No.	Time (min)	Pct A
Profile:	1	0	100

Flow Rate: 1 mL/min

Col. Temp.: ambient


Detection: UV-Vis Abs.-Variable Wave.(UV) @ 280 nm (ambient)

Analyst Note: SecurityGuard[™] Guard Cartridge System extends column lifetime.


- SecurityGuard Cartridges, GFC-2000 4 x 3.0mm ID, 10/Pk Part No.: AJ0-4487

- Holder Part No.: KJ0-4282

19806



Products used in this application:

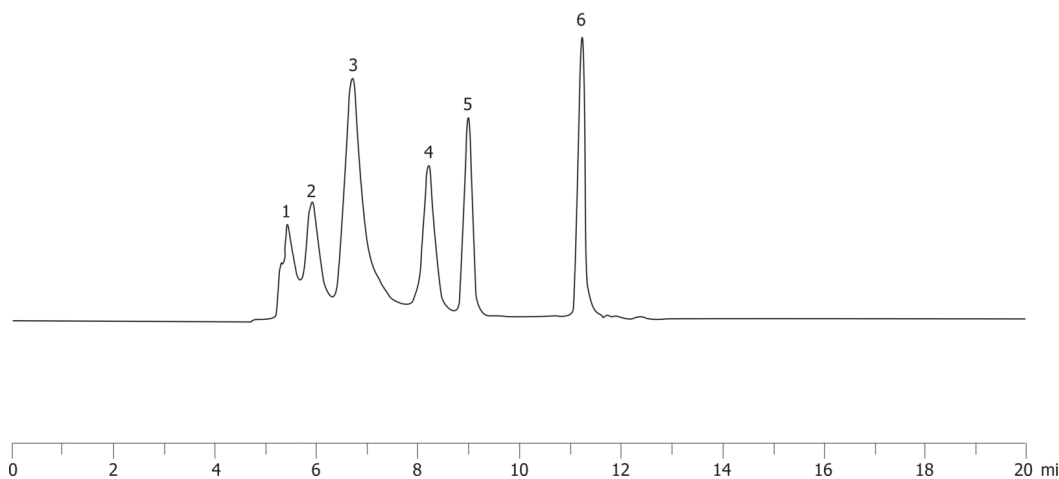

ANALYTES:

- 1** Bovine Thyroglobulin
Retention Time: 5.3 min
- 2** IgA
Retention Time: 5.93 min
- 3** IgG
Retention Time: 6.7 min
- 4** Ovalbumin
Retention Time: 8.21 min
- 5** Myoglobin
Retention Time: 9 min
- 6** Uridine
Retention Time: 11.23 min

