

## Underivatized MMA and Succinic Acid in Human Urine on Gemini C18, 3u, 100x3 mm

**Column:** Gemini® 3 µm C18 110 Å, LC Column 100 x 3 mm, Ea  
**Dimensions:** 100 x 3 mm ID  
**Order No:** 00D-4439-Y0  
**Elution Type:** Gradient  
**Eluent A:** 0.1% Formic Acid in DI H2O  
**Eluent B:** 0.1% Formic Acid + 10 mM Ammonium Formate in MeOH

| Gradient Profile: | Step No. | Time (min) | Pct A | Pct B |
|-------------------|----------|------------|-------|-------|
|                   | 1        | 0          | 85    | 15    |
|                   | 2        | 1.5        | 5     | 95    |
|                   | 3        | 2.5        | 5     | 95    |
|                   | 4        | 2.51       | 85    | 15    |
|                   | 5        | 4.5        | 85    | 15    |

**Flow Rate:** 700 µL/min  
**Col. Temp.:** 40 °C  
**Detection:** Tandem Mass Spec (MS-MS) @ (ambient)


**Detector Info:** <a target="\_blank"

**Analyst Note:** href="https://sciex.com/products/mass-spectrometers?utm\_campaign=2019%20application%20search&utm\_source=phenomenex&utm\_medium=referral">SCIEX<br/>SecurityGuard™ Guard Cartridge System extends column lifetime.

- SecurityGuard Cartridges, Gemini C18 4 x 2.0mm ID, 10/PK Part No.: AJ0-7596
- Holder Part No.: KJ0-4282



Products used in this application:

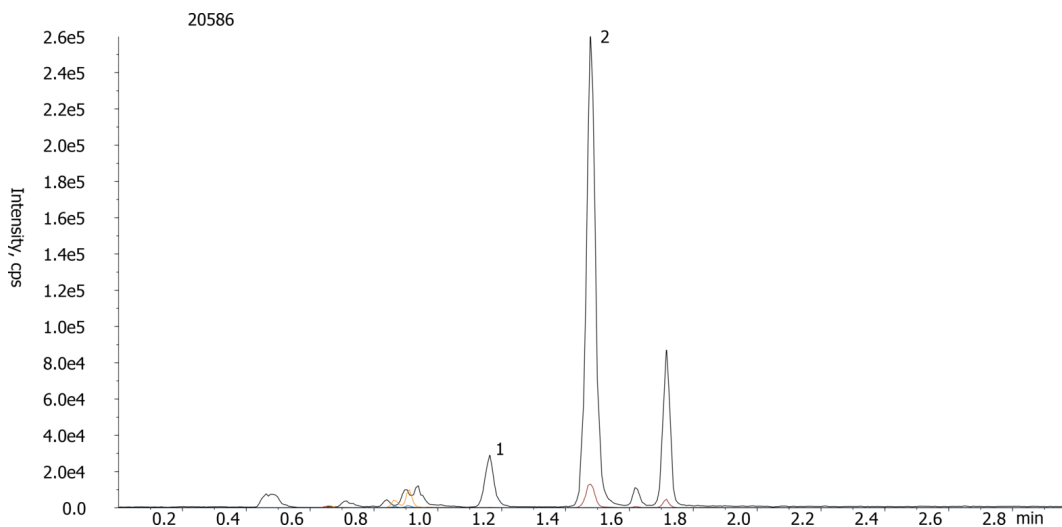

### ANALYTES:

- 1 Succinic acid  
Retention Time: 1.16 min
- 2 Methylmalonic acid  
Retention Time: 1.48 min



# Sample Preparation Details

for HPLC Application ID No.: 20586

## Underivatized MMA and Succinic Acid in Human Urine on Gemini C18, 3u, 100x3 mm

### PRODUCT DESCRIPTION:

Strata™-X-AW 33 µm Polymeric Weak Anion, 30 mg / 1 mL, Tubes , 100/Pk

Order No.: 8B-S038-TAK

### SOLID PHASE EXTRACTION (SPE) PROCEDURE:

**Note:** The solvent volumes shown below are for a 30 mg bed mass.

The solvent volumes will need to be adjusted for a smaller or larger bed mass.

#### Condition:

---

#### Load:

---

Into individually labeled 1.5 mL conical micro-centrifuge tubes combine 0.5 mL 25 mM Ammonium formate, 50 µL IS and 100 µL blank, standard, or sample

#### Wash:

---

#### Dry:

---

Dry under high vacuum for 5-10 min

#### Elute:

---

### Final Prep and Analysis:

---

This method is for the analysis of underivatized MMA.

Inject: 10 µL on HPLC Tandem Mass Spec (MS-MS) @ (ambient)

| ANALYTES:            | Spiked Conc.<br>(ng/mL) | Log P | pKa | % Rec | %RSC<br>(n=0) |
|----------------------|-------------------------|-------|-----|-------|---------------|
| 1 Succinic acid      | 0                       |       |     |       |               |
| 2 Methylmalonic acid | 0                       |       |     |       |               |

**Note:** This method is designed as a convenient starting point for further investigation and can be tailored to meet your extraction goals. Call your local Phenomenex Representative for assistance in method development and optimization techniques.

©2024 Phenomenex Inc. All rights reserved.

For more information contact your Phenomenex Representative at support@phenomenex.com



Phenomenex products are available worldwide.

[www.phenomenex.com](http://www.phenomenex.com)

[support@phenomenex.com](mailto:support@phenomenex.com)