

## Pain Panel using Strata-X-Drug B and Kinetex Phenyl-Hexyl 2.6u 50x4.6mm

**Column:** Kinetex® 2.6 µm Phenyl-Hexyl 100 Å, LC Column 50 x 4.6 mm, Ea

**Dimensions:** 50 x 4.6 mm ID

**Order No:** 00B-4495-E0

**Elution Type:** Gradient

**Eluent A:** 10mM ammonium formate

**Eluent B:** 0.1% Formic acid/methanol

Gradient Profile:	Step No.	Time (min)	Pct A	Pct B
	1	0	95	5
	2	4	0	100
	3	5	0	100
	4	5.1	95	5
	5	7	95	5

**Flow Rate:** 0.6 mL/min

**Col. Temp.:** ambient

**Detection:** Mass Spectrometer (MS) @ amu (ambient)

**Detector Info:** <a target="\_blank"

**Analyst Note:**


href="https://sciex.com/products/mass-spectrometers?utm\_campaign=2019%20application%20search&utm\_source=phenomenex&utm\_medium=referral">SCIEX<

MS/MS Parameters

Detection: API 5000 MS/MS, TurboIonspray, positive polarity  
CAD Gas: 7; GS1, GS2 = 50; curtain gas: 20, ESI spray voltage: 5500; Temp: 650 deg C



Products used in this application:

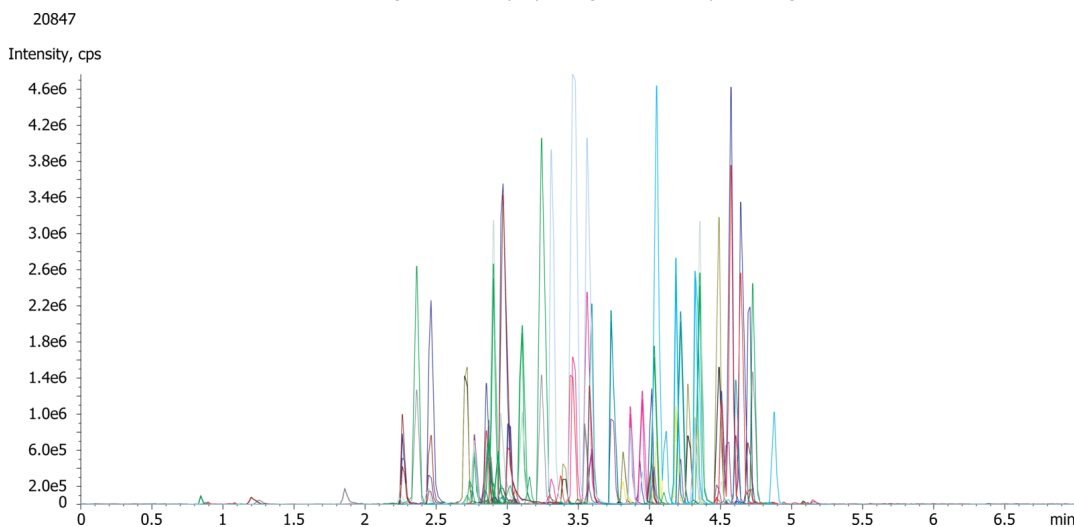

## Pain Panel using Strata-X-Drug B and Kinetex Phenyl-Hexyl 2.6u 50x4.6mm

### ANALYTES:

<b>1</b> Morphine	<b>41</b> Methadone
<b>2</b> Morphine-d6	<b>42</b> Methadone-d3
<b>3</b> Hydromorphone	<b>43</b> Midazolam
<b>4</b> Hydromorphone-d6	<b>44</b> Lorazepam
<b>5</b> Naloxone	<b>45</b> Clonazepam
<b>6</b> Codeine	<b>46</b> Hydroxyalprazolam
<b>7</b> Oxymorphone	<b>47</b> Oxazepam
<b>8</b> Naltrexone	<b>48</b> Flunitrazepam
<b>9</b> Amphetamine	<b>49</b> Alprazolam
<b>10</b> Amphetamine-d5	<b>50</b> Temazepam
<b>11</b> 6-MAM	<b>51</b> Nordiazepam
<b>12</b> Oxycodone	<b>52</b> Nordiazepam-d5
<b>13</b> Hydrocodone	<b>53</b> Diazepam
<b>14</b> Hydrocodone-d6	<b>54</b> 6-MAM-d3
<b>15</b> Methamphetamine	<b>55</b> Methamphetamine-d5
<b>16</b> MDA	
<b>17</b> MDMA	
<b>18</b> MDEA	
<b>19</b> Norfentanyl	
<b>20</b> Tramadol	
<b>21</b> Benzoylcegonine	
<b>22</b> Benzoylcegonine-d3	
<b>23</b> Meperidine	
<b>24</b> Meperidine-d4	
<b>25</b> Normeperidine	
<b>26</b> Normeperidine-d4	
<b>27</b> Meprobamate	
<b>28</b> Norbuprenorphine	
<b>29</b> PCP	
<b>30</b> PCP-D5	
<b>31</b> Fentanyl	
<b>32</b> Fentanyl-d5	
<b>33</b> EDDP	
<b>34</b> Flurazepam	
<b>35</b> Norpropoxyphene	
<b>36</b> Norpropoxyphene-d5	
<b>37</b> Sufentanil	
<b>38</b> Buprenorphine	
<b>39</b> Propoxyphene	
<b>40</b> Carisoprodol	



# Sample Preparation Details

for HPLC Application ID No.: 20847

## Pain Panel using Strata-X-Drug B and Kinetex Phenyl-Hexyl 2.6u 50x4.6mm

### PRODUCT DESCRIPTION:

Strata<sup>™</sup>-X-Drug B 33 µm Polymeric Strong Cation, 30 mg / 3 mL, Tubes , 50/Pk

Order No.: 8B-S128-TBJ

### SOLID PHASE EXTRACTION (SPE) PROCEDURE:

**Note:** The solvent volumes shown below are for a 30 mg bed mass.

The solvent volumes will need to be adjusted for a smaller or larger bed mass.

### Condition:

---

### Load:

---

Sample Hydrolysis: Measure 200µL Urine (calibrator, control) in a 1.5mL micro centrifuge tube, add 20 µL combined IS (Internal Standard) spiking solution.

Vortex 10-15 secs followed by adding 100µL 0.1M pH 4.0 ammonium acetate buffer to each tube, mix/vortex another 15 secs.

Add 40µL

beta-Glucuronidase solution (100,000 units/mL).

Vortex 10-15 secs.

Incubate for 2 hours in a shaker at 55o C to complete hydrolysis of the glucuronides.

Add 400µl of 0.1% FA (formic acid) followed by vortexing for another 60 secs.

Centrifuge the hydrolyzed samples at appx 21000 g for 10 mins (to separate any proteins). Collect Supernatant

### Wash:

---

### Dry:

---

3 to 4 mins at high vacuum (10" of Hg)

### Elute:

---

### Final Prep and Analysis:

---

Load: Samples from hydrolysis Using b-Glucuronidase as below

To 200 µL Urine (calibrator, control) in a 1.5 mL micro centrifuge tube, add 20 µL combined IS

Inject: 10 µL on HPLC Mass Spectrometer (MS) @ amu (ambient)

<b>ANALYTES:</b>	<b>Spiked Conc.</b> <b>(ng/mL)</b>	<b>Log P</b>	<b>pKa</b>	<b>% Rec</b>	<b>%RSC</b> <b>(n=0)</b>
<b>1</b> Morphine	25			115	
<b>2</b> Morphine-d6	500				
<b>3</b> Hydromorphone	25			110	
<b>4</b> Hydromorphone-d6	500				
<b>5</b> Naloxone	25			103	
<b>6</b> Codeine	25			111	
<b>7</b> Oxymorphone	25			107	
<b>8</b> Naltrexone	25			108	
<b>9</b> Amphetamine	125			99	
<b>10</b> Amphetamine-d5	2500				
<b>11</b> 6-MAM	2.5			99	
<b>12</b> Oxycodone	25			113	
<b>13</b> Hydrocodone	25			113	
<b>14</b> Hydrocodone-d6	312				
<b>15</b> Methamphetamine	125			113	
<b>16</b> MDA	62.5			99	



# Sample Preparation Details

for HPLC Application ID No.: 20847

## Pain Panel using Strata-X-Drug B and Kinetex Phenyl-Hexyl 2.6u 50x4.6mm

<b>ANALYTES (cont.):</b>	<b>Spiked Conc. (ng/mL)</b>	<b>Log P</b>	<b>pKa</b>	<b>% Rec</b>	<b>%RSC (n=0)</b>
17 MDMA	62.5			102	
18 MDEA	62.5			104	
19 Norfentanyl	2.5			112	
20 Tramadol	25			96	
21 Benzoylecgonine	37.5			100	
22 Benzoylecgonine-d3	750				
23 Meperidine	250			95	
24 Meperidine-d4	3000				
25 Normeperidine	25			108	
26 Normeperidine-d4	500				
27 Meprobamate	50			108	
28 Norbuprenorphine	25			93	
29 PCP	6.25			120	
30 PCP-D5	125				
31 Fentanyl	0.75			110	
32 Fentanyl-d5	100				
33 EDDP	25			113	
34 Flurazepam	25			117	
35 Norpropoxyphene	37.5			103	
36 Norpropoxyphene-d5	750				
37 Sufentanil	0.75			84	
38 Buprenorphine	25			100	
39 Propoxyphene	37.5			98	
40 Carisoprodol	50			112	
41 Methadone	25			101	
42 Methadone-d3	500				
43 Midazolam	25			114	
44 Lorazepam	25			102	
45 Clonazepam	25			117	
46 Hydroxyalprazolam	25			111	
47 Oxazepam	25			99	
48 Flunitrazepam	25			98	
49 Alprazolam	25			101	
50 Temazepam	25			104	
51 Nordiazepam	25			110	
52 Nordiazepam-d5	500				
53 Diazepam	25			114	
54 6-MAM-d3	500				
55 Methamphetamine-d5	2500				

**Note:** This method is designed as a convenient starting point for further investigation and can be tailored to meet your extraction goals. Call your local Phenomenex Representative for assistance in method development and optimization techniques.

©2025 Phenomenex Inc. All rights reserved.

For more information contact your Phenomenex Representative at [support@phenomenex.com](mailto:support@phenomenex.com)



Phenomenex products are available worldwide.

[www.phenomenex.com](http://www.phenomenex.com)

[support@phenomenex.com](mailto:support@phenomenex.com)