

## Calibration Curve: Yarra 3µm SEC-3000 Standard with different salt MP


**Column:** Yarra™ 3 µm SEC-3000, LC Column 300 x 7.8 mm, Ea  
**Dimensions:** 300 x 7.8 mm ID  
**Order No:** 00H-4513-K0  
**Elution Type:** Isocratic  
**Eluent A:** 50 mM Sodium Phosphate in Water pH 6.8 with 0.025% NaN<sub>3</sub>  
**Gradient**

Step No.	Time (min)	Pct A
1	0	100

**Profile:**  
**Flow Rate:** 1 mL/min  
**Col. Temp.:** ambient  
**Detection:** UV-Vis Abs.-Variable Wave.(UV) @ 280 nm (ambient)



Products used in this application:

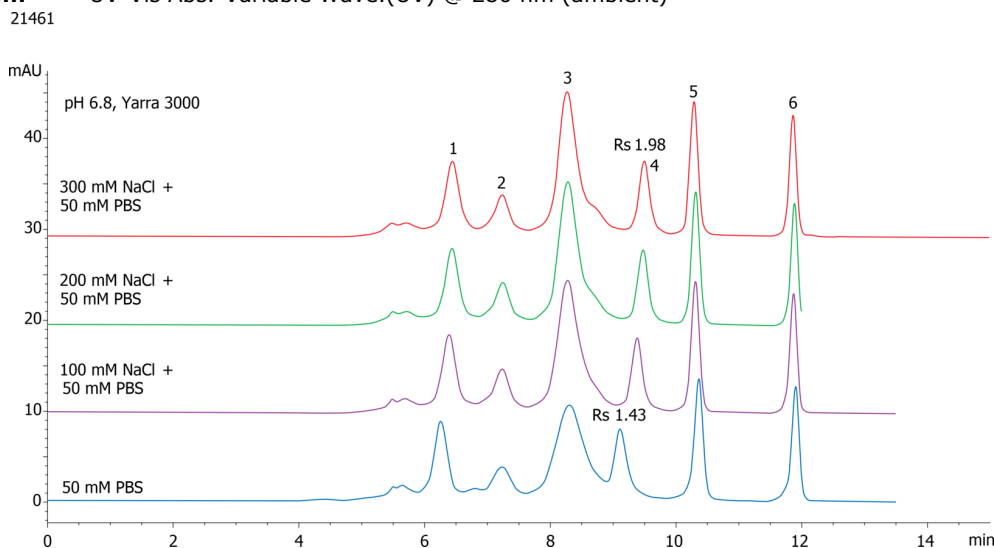

### ANALYTES:

- 1** Thyroglobulin  
Retention Time: 6 min
- 2** IgA  
Retention Time: 6.7 min
- 3** IgG  
Retention Time: 7.7 min
- 4** Ovalbumin  
Retention Time: 9.2 min
- 5** Myoglobin  
Retention Time: 9.8 min
- 6** Uridine  
Retention Time: 11.5 min

