

# HPLC Application

ID No.: 22747

## Aeris Ig-G comparison widepore XB-C18

**Column:** Aeris™ 3.6 µm WIDEPORE XB-C18 200 Å, LC Column 150 x 4.6 mm, Ea

**Dimensions:** 150 x 4.6 mm ID

**Order No:** 00F-4482-E0

**Elution Type:** Gradient

**Eluent A:** 0.1% TFA

**Eluent B:** 0.085% TFA in AcCN



Gradient Profile:	Step No.	Time (min)	Pct A	Pct B
	1	0	90	10
	2	1	80	20
	3	15	40	60
	4	15.01	90	10

**Flow Rate:** 1

**Col. Temp.:** 40 °C

**Detection:** UV-Vis Abs.-Variable Wave.(UV) @ 214 nm (ambient)

22747

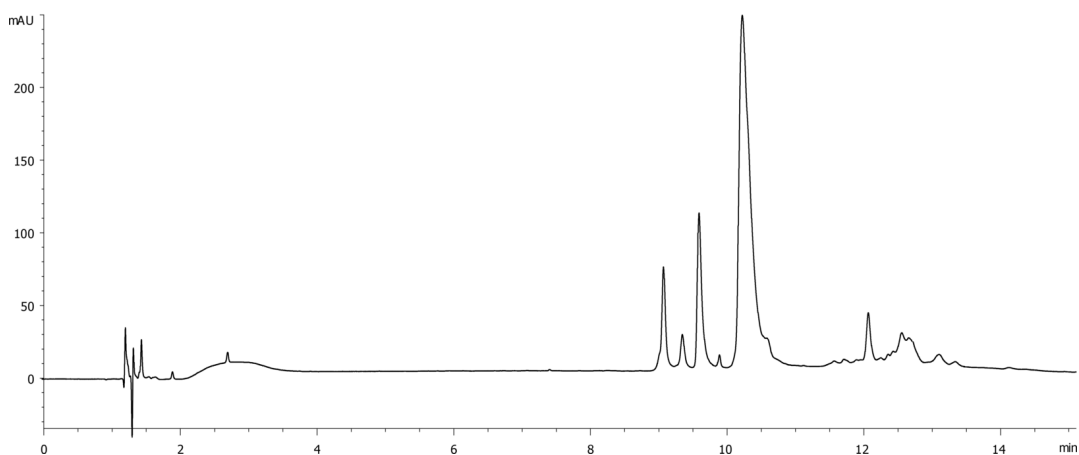

Products used in this application:



### ANALYTES:

- 1 Ig-G1 Standard

