

HPLC Application

ID No.: 23218

Degraded Human Insulin on Yarra 1.8 µm SEC-X150

Column: N/A

Dimensions: N/A

Order No: N/A

Elution Type: N/A

Eluent A: 1g/L L-Arginine in water

Eluent B: Acidic Acid


Eluent C: Acetonitrile

Gradient Profile:	Step No.	Time (min)	Pct A	Pct B	Pct C
	1	0	65	15	20

Flow Rate: 0.2 mL/min

Col. Temp.: ambient

Detection: UV-Vis Abs.-Diode Array (PDA) @ 276 nm (ambient)

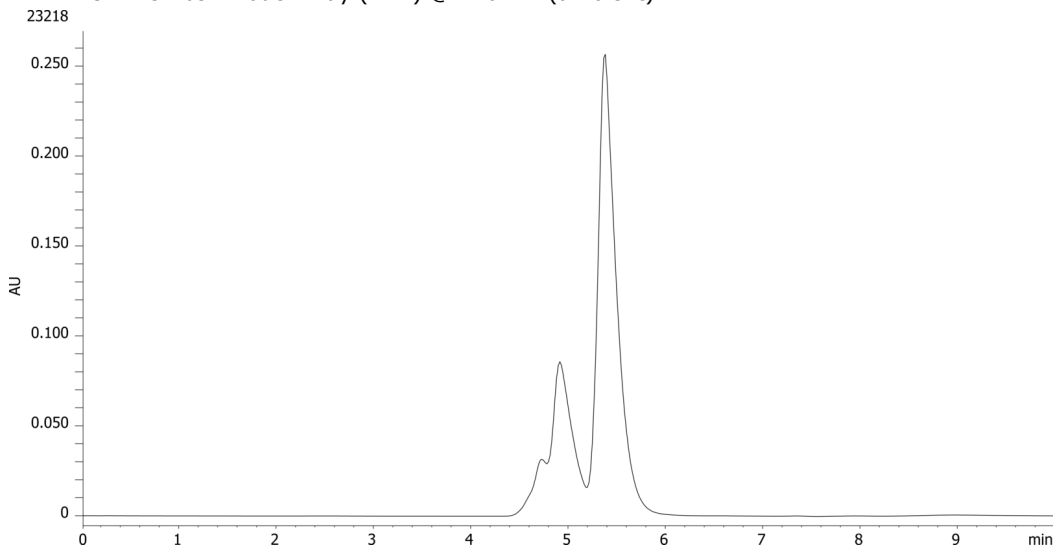

ANALYTES:

- 1** Aggregates
Retention Time: 4.735 min
- 2** Aggregates
Retention Time: 4.919 min
- 3** Insulin
Retention Time: 5.38 min