


Yarra 1.8 µm SEC-X150 Lifetime and Stability, 100 hours at 0.4 mL/min

Column: N/A
Dimensions: N/A
Order No: N/A
Elution Type: N/A
Eluent A: 10% IPA
Gradient
Profile:

Step No.	Time (min)	Pct A
1	0	100

Flow Rate: 0.4 mL/min
Col. Temp.: ambient
Detection: UV-Vis Abs.-Variable Wave.(UV) @ 280 nm (ambient)

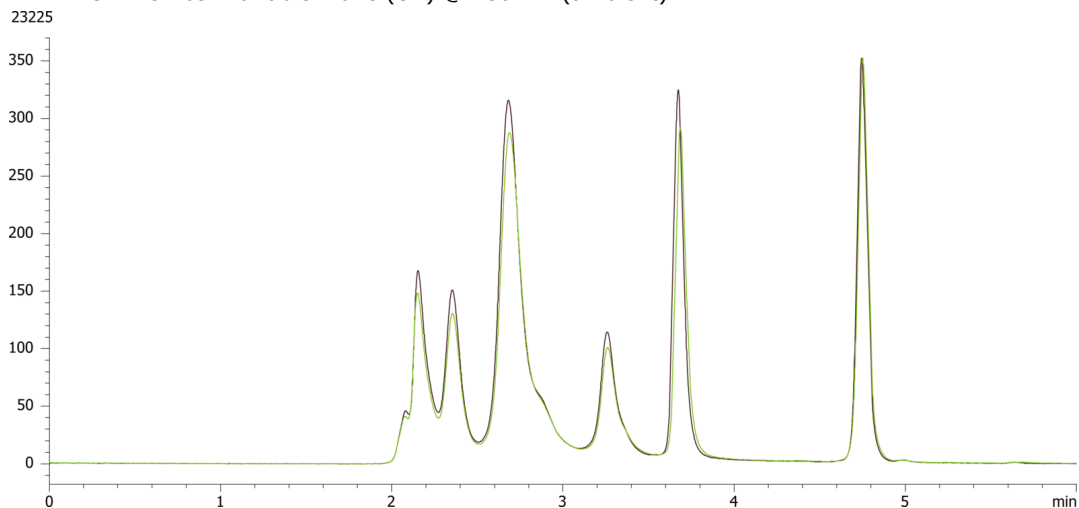

ANALYTES:

- 1** Thyroglobulin
Retention Time: 2.152 min
- 2** IgA
Retention Time: 2.35 min
- 3** IgG
Retention Time: 2.682 min
- 4** Ovalbumin
Retention Time: 3.26 min
- 5** Myoglobin
Retention Time: 3.686 min
- 6** Uridine
Retention Time: 4.754 min

