


Yarra 1.8 μ m SEC-X150 Batch-to-Batch Reproducibility

Column: N/A
Dimensions: N/A
Order No: N/A
Elution Type: N/A
Eluent A: 0.1 M Sodium Phosphate, pH 6.8
Gradient

Step No.	Time (min)	Pct A
1	0	100

Profile:
Flow Rate: 0.3 mL/min
Col. Temp.: ambient
Detection: UV-Vis Abs.-Variable Wave.(UV) @ 280 nm (ambient)

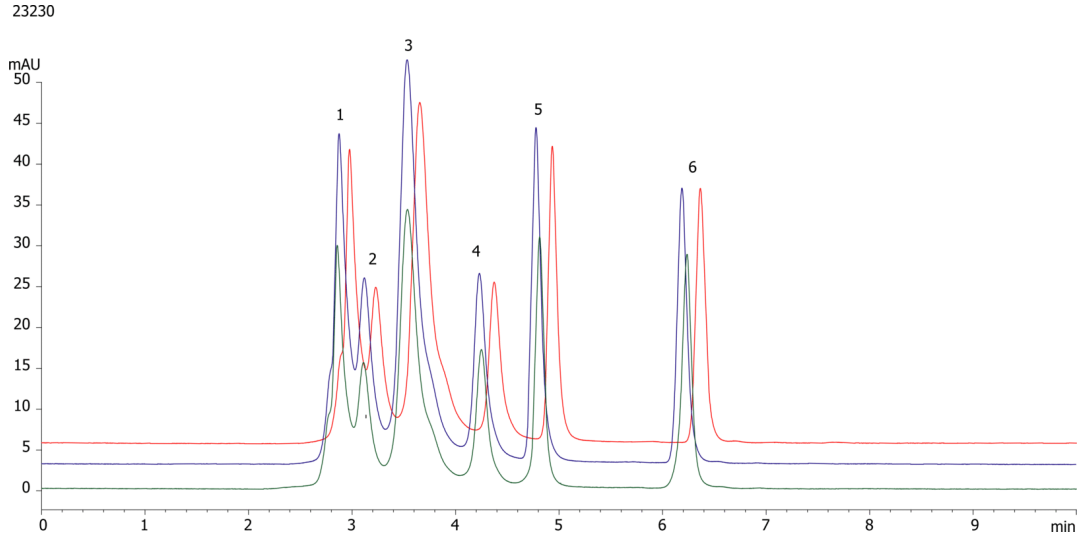

ANALYTES:

- 1 Thyroglobulin
- 2 IgA
- 3 IgG
- 4 Ovalbumin
- 5 Myoglobin
- 6 Uridine

