


## Yarra 1.8 µm SEC-X150, Test Mix

**Column:** N/A  
**Dimensions:** N/A  
**Order No:** N/A  
**Elution Type:** N/A  
**Eluent A:** 0.1 M Sodium Phosphate, pH 6.8  
**Gradient**  

Step No.	Time (min)	Pct A
1	0	100

  
**Profile:**  
**Flow Rate:** 0.3 mL/min  
**Col. Temp.:** ambient  
**Detection:** UV-Vis Abs.-Variable Wave.(UV) @ 280 nm (ambient)

23243

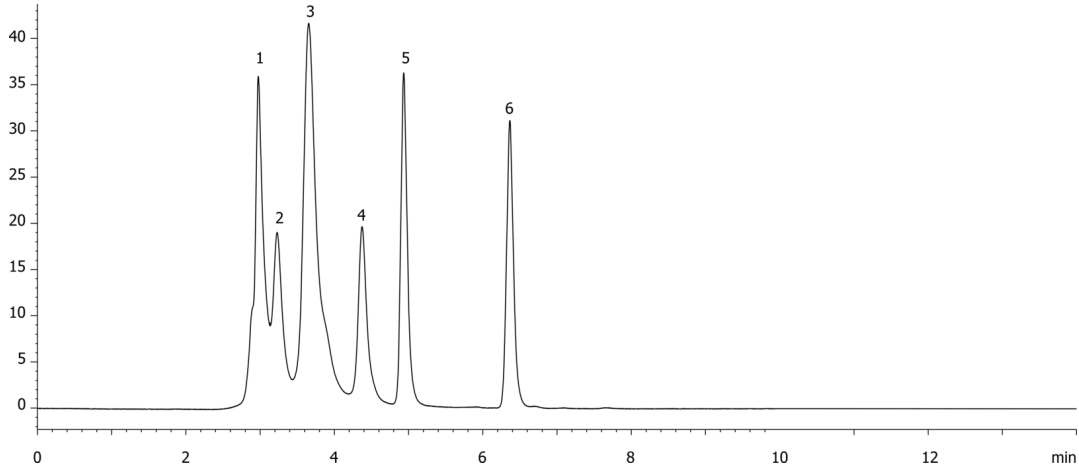

### ANALYTES:

- 1** Thyroglobulin  
Retention Time: 2.976 min
- 2** IgA  
Retention Time: 3.229 min
- 3** IgG  
Retention Time: 3.654 min
- 4** Ovalbumin  
Retention Time: 4.373 min
- 5** Myoglobin  
Retention Time: 4.934 min
- 6** Uridine  
Retention Time: 6.364 min

