


Yarra 1.8 μ m SEC-X150, Test Mix

Column: N/A
Dimensions: N/A
Order No: N/A
Elution Type: N/A
Eluent A: 0.1 M Sodium Phosphate, pH 6.8
Gradient

Step No.	Time (min)	Pct A
1	0	100

Profile:
Flow Rate: 0.3 mL/min
Col. Temp.: ambient
Detection: UV-Vis Abs.-Variable Wave.(UV) @ 280 nm (ambient)

23243

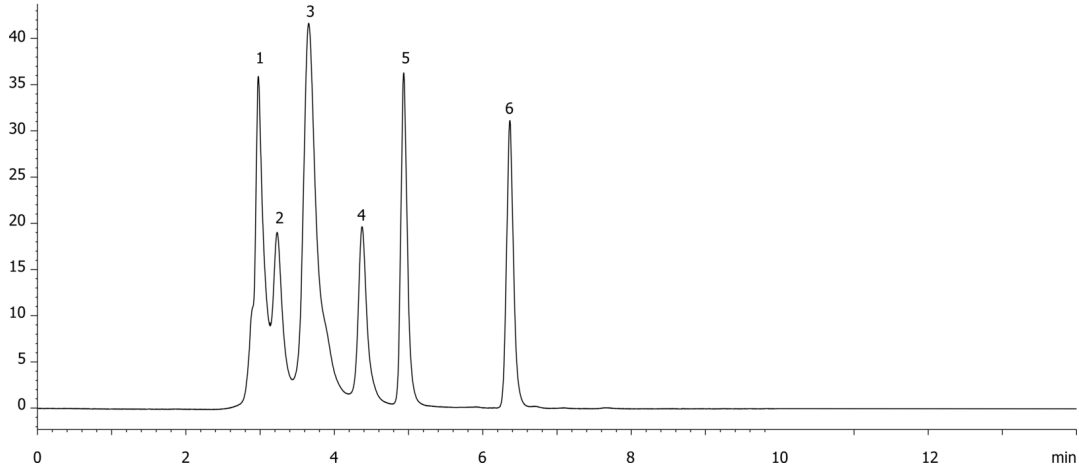

ANALYTES:

- 1** Thyroglobulin
Retention Time: 2.976 min
- 2** IgA
Retention Time: 3.229 min
- 3** IgG
Retention Time: 3.654 min
- 4** Ovalbumin
Retention Time: 4.373 min
- 5** Myoglobin
Retention Time: 4.934 min
- 6** Uridine
Retention Time: 6.364 min

