HPLC Application

ID No.: **8713**

Estradiol - USP Acceptable Modified Method

Products used in this application:

LUNA®

Column:	Luna® 5 µm C18(2) 100 Å, LC Column 250 x 4.6 mm, Ea			
Dimensions:	250 x 4.6 mm ID			
Order No:	00G-4252-E0			
Elution Type:	Isocratic			
Eluent A:	Acetonitrile			
Eluent B:	Water			
Gradient	**Step No.**	**Time (min)**	**Pct A**	**Pct B**
Profile:	**1**	0	55	45
Flow Rate:	1 mL/min			
Col. Temp.:	ambient			
Detection:	UV-Vis Abs.-Variable Wave.(UV) @ 205 nm (ambient)			
Analyst Note:	SecurityGuard™ Guard Cartridge System extends column lifetime.			

- SecurityGuard Cartridges, C18 4 x 3.0mm, 10/Pk Part No.: AJ0-4287
- Holder Part No.: KJ0-4282

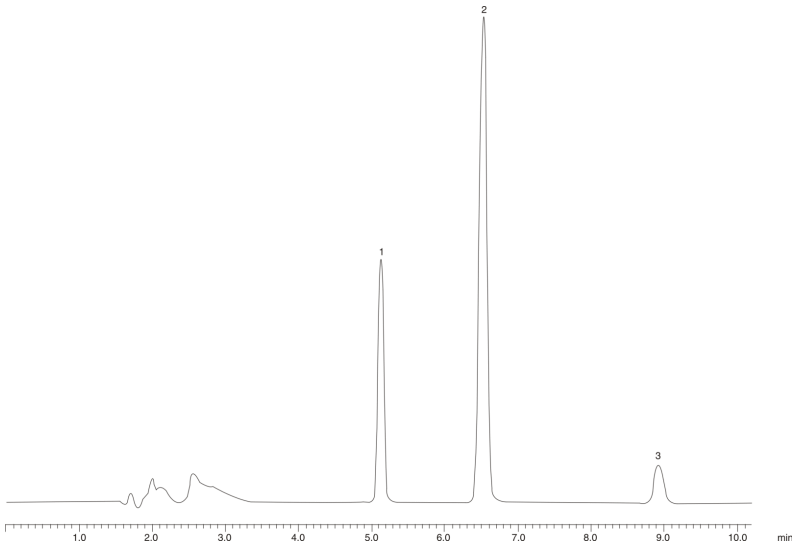

ANALYTES:

1. Ethyl paraben
2. Estradiol
3. Estrone

©2024 Phenomenex Inc. All rights reserved.

For more information contact your Phenomenex Representative at support@phenomenex.com

Phenomenex products are available worldwide.